

KoolAir Ankle w/ Valve

Application Instructions

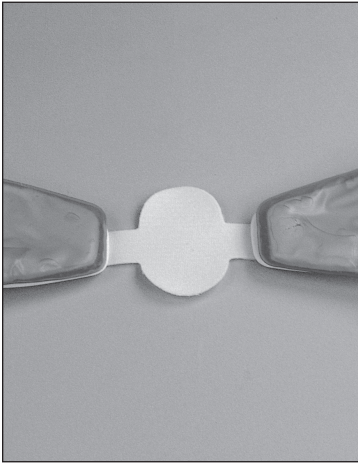


Figure 1 - Open ankle stirrup

⚠ Caution:

- Patients should always consult their physician or therapist for proper therapy instructions prior to using the therapeutic ankle support.
- Always wear a cotton sock before cold therapy is applied.

1. Open ankle stabilizer and lay flat.
2. Position the heel evenly on the center pad.
3. Wrap the lower hook and loop closure strap around the ankle for alignment. Center the side shells along the ankle and the leg. Wrap the upper strap and adjust if necessary.
4. Tighten lower and upper straps for a secure fit and for patient comfort.
5. Adjust the vertical side straps, placing both hands on straps, pulling upward until desired fit.
6. Secure vertical side straps with hook and loop closure.

KoolAir Ankle Fit Adjustment - The KoolAir Ankle is pre-inflated and should not need to be inflated further. However, if you experience discomfort you may try these things: 1) Reposition the stabilizer and/or readjust other components; or 2) Adjust air volume (keep in mind too much air will take away support).

To Add Air - Insert the tube into opening and blow into tube, squeeze valve just below the tube and remove tube.

To Remove Air - Squeeze bladder and squeeze valve.

High Altitude - High altitudes will cause bladder to expand and you will have to remove air. Readjust the straps when flying for comfort.

Note: *The KoolAir Ankle should always be worn over a cotton sock. Consult your physician for further instruction on application and treatment*

Note: Outer shell may be wiped with mild soap and water.



Manufactured For:

Breg, Inc.
 2885 Loker Ave. East
 Carlsbad, CA 92010 U.S.A.
 P: 800-321-0607
 F: 800-329-2734
 www.breg.com
 AW-1.00294 Rev B 1012



Figure 4 - Tighten lower and upper straps



Figure 2 - Position heel on center pad



Figure 5 - Adjust vertical side straps

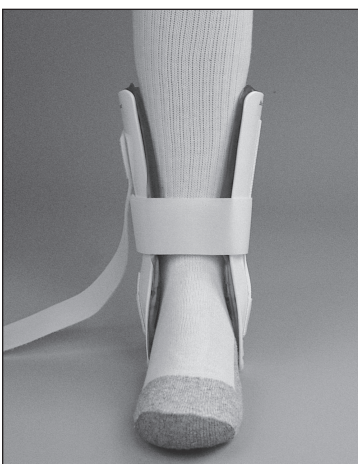


Figure 3 - Center side shells along ankle and leg



Figure 6 - Secure straps

Made in USA